Excellentcare Medical (Huizhou) Ltd.
Shatou Industrial Zone, Yuanzhou Town, Boluo County,
Huizhou, 516123, Guangdong, China
Tel: 0752-6358333 Fax: 0752-6358899
E-Mail: info@excellentcare.com.cn

Emedical®
Total Excellent-Total Care

Revision date: 25/12/2023
Revision number: 00/ Dec 2023

Breathing Circuit

Instructions for Use

REF EM07-003

Intended use:

Breathing Circuit is used to transfer gas between patient and ventilator.

Structure and Components:

The device consists of suction connector, corrugated tube, machine end adaptor. The assembly drawing is illustrated as follows:

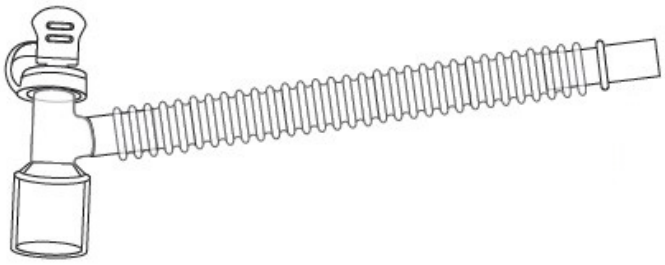

Directions for Use:

1. Wash and dry your hands.
2. Before use, visually observe all components to ensure that there is no defacement and damage.
3. Connect the breathing circuit machine end to the ventilator intake and outlet port.
4. Connect the machined end of this product to the Y-piece of the breathing circuit.
5. Connect the suction connector of this product to the endotracheal tube, mask or other breathing device directly or by some connection accessories.

Note: In order to alleviate the discomfort caused by the Y-piece being too close to the patient's face and the operational difficulties for the medical staff, the product with the double swivel elbow can be connected to the Y-piece to extend the breathing circuit.

Contra-indications:

None

Transport and Storage:

Keep away from high pressure and sunlight and keep dry during transportation. The storage conditions: relative humidity should be less than 80%, shady and cool, dry, clean, draughty, no corrosive gas.

Precautions:

1. Do not use if the device is damaged or the unit packaging is damaged or opened.
2. Do not use if product is beyond the date of expiry.
3. For single patient use only.

4. It is recommended that the use period of the breathing circuit is 7 days. If the circuit is seriously polluted, new one should be replaced immediately.
5. Please pay attention on the airtightness of breathing circuit, such as air leakage, please find out the cause immediately and deal with it in time

Warnings:

1. Do not reuse, reprocess, or re-sterilize this medical device. Reuse, reprocessing, or re-sterilization may:
    a. adversely affect the known biocompatibility characteristics of the device
    b. compromise the structural integrity of the device
    c. lead to the device not performing as intended
    d. create a risk of contamination and cause the transmission of infectious diseases resulting in patient injury, illness, or death

2. The used product should be properly disposed according to the local legislations.

Legal manufacturer:

Global SCP Medical Systems Pte. Ltd., Singapore

Excellentcare Medical (Huizhou) Ltd.
Shatou Industrial Zone, Yuanzhou Town, Boluo County,
Huizhou, 516123, Guangdong, China
Tel: 0752-6358333 Fax: 0752-6358899
E-Mail: info@excellentcare.com.cn

Emedical®
Total Excellent-Total Care

Revision date: 25/12/2023
Revision number: 00/ Dec 2023

Breathing Circuit

Instructions for Use

REF EM07-004

Intended use:

Breathing Circuit is used to transfer gas between patient and ventilator.

Structure and Components:

The device consists of suction connector, expandable corrugated tube, machine end adaptor. The assembly drawing is illustrated as follows:

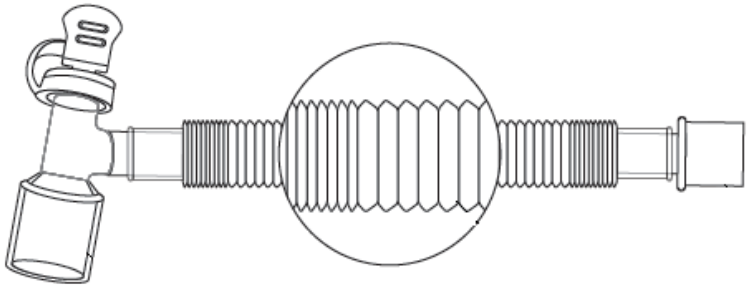

Directions for Use:

1. Wash and dry your hands.

2. Before use, visually observe all components to ensure that there is no defacement and damage.

3. Connect the breathing circuit machine end to the ventilator intake and outlet port.

4. Connect the machined end of this product to the Y-piece of the breathing circuit.

5. Connect the suction connector of this product to the endotracheal tube, mask or other breathing device directly or by some connection accessories.

Note: In order to alleviate the discomfort caused by the Y-piece being too close to the patient's face and the operational difficulties for the medical staff, the product with the double swivel elbow can be connected to the Y-piece to extend the breathing circuit.

Contra-indications:

None

Transport and Storage:

Keep away from high pressure and sunlight and keep dry during transportation. The storage conditions: relative humidity should be less than 80%, shady and cool, dry, clean, draughty, no corrosive gas.

Precautions:

1. Do not use if the device is damaged or the unit packaging is damaged or opened.
2. Do not use if product is beyond the date of expiry.
3. For single patient use only.

4. It is recommended that the use period of the breathing circuit is 7 days. If the circuit is seriously polluted, new one should be replaced immediately.
5. Please pay attention on the airtightness of breathing circuit, such as air leakage, please find out the cause immediately and deal with it in time

Warnings:

1. Do not reuse, reprocess, or re-sterilize this medical device. Reuse, reprocessing, or re-sterilization may:
    a. adversely affect the known biocompatibility characteristics of the device
    b. compromise the structural integrity of the device
    c. lead to the device not performing as intended
    d. create a risk of contamination and cause the transmission of infectious diseases resulting in patient injury, illness, or death

2. The used product should be properly disposed according to the local legislations.

Legal manufacturer:

Global SCP Medical Systems Pte. Ltd., Singapore

Excellentcare Medical (Huizhou) Ltd.
Shatou Industrial Zone, Yuanzhou Town, Boluo County,
Huizhou, 516123, Guangdong, China
Tel: 0752-6358333 Fax: 0752-6358899
E-Mail: info@excellentcare.com.cn

Emedical®
Total Excellent-Total Care

Revision date: 25/12/2023
Revision number: 00/ Dec 2023

Breathing Circuit

Instructions for Use

REF S05-110

Intended use:

Breathing Circuit is used to transfer gas between patient and ventilator. This breathing circuit accessory is an exhalation connector, it is used to connect the non-invasive mask and breathing circuit for exhalation.

Structure and Components:

The assembly drawing is illustrated as follows:



Directions for Use:

1. Wash and dry your hands.
2. Connect the exhalation connector to the patient end of breathing tube.
3. Connect the exhalation connector to the non-invasive mask or other breathing device directly.

Contra-indications:

None

Transport and Storage:

Keep away from high pressure and sunlight and keep dry during transportation. The storage conditions: relative humidity should be less than 80%, shady and cool, dry, clean, draughty, no corrosive gas.

Precautions:

1. Do not use if the device is damaged or the unit packaging is damaged or opened.
2. Do not use if product is beyond the date of expiry.
3. For single patient use only.
4. It is recommended that the use period of the breathing circuit is 7 days. If the circuit is seriously polluted, new one should be replaced immediately.
5. Please pay attention on the exhalation of connector, please find out the cause immediately and deal with it in time.

Warnings:

1. Do not reuse, reprocess, or re-sterilize this medical device. Reuse, reprocessing, or re-sterilization may:
    a. adversely affect the known biocompatibility characteristics of the device
    b. compromise the structural integrity of the device
    c. lead to the device not performing as intended
    d. create a risk of contamination and cause the transmission of infectious diseases resulting in patient injury, illness, or death

2. The used product should be properly disposed according to the local legislations.

Legal manufacturer:

Global SCP Medical Systems Pte. Ltd., Singapore