Excellentcare Medical (Huizhou) Ltd.
Shatou Industrial Zone, Yuanzhou Town, Boluo County,
Huizhou, 516123, Guangdong, China
Tel: 0752-6358333 Fax: 0752-6358899
E-Mail: info@excellentcare.com.cn

Emedical®
Total Excellent-Total Care

Urine Drainage Bag
Instructions for Use

Revision date: 25/12/2023
Revision number: 00/ Dec 2023


REF EM33-102

Intended use:

Urine drainage bag with scale for collection and monitoring of urine output.

Structure and Components:

The device consists of consists of inlet tubing, non-return valve, urine tank, urine drainage bag, drainage tap and hanger. The assembly drawing is illustrated as follows:

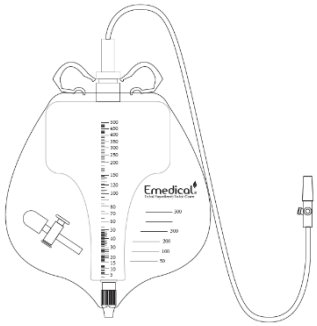

Directions for Use:

1. Adjust the patient position and expose the connector of the urinary catheter. (Note: Before connecting the urine drainage bag, you need to insert the urinary catheter into the patient first, and use the hemostatic forceps to block the urinary catheter to prevent urine from flowing out.)
2. Open the package, ensure the drainage tap is closed, then hang the hanger of urine drainage bag on the bedside.
3. Open the cap on the connector of the inlet tubing, and connect to the urinary catheter, after finishing, loosen the hemostatic forceps.
4. Place the patient in a comfortable position.
5. When the urine tank is filled with urine, raise the urine tank to a certain height and the urine flow to the bag; it can also naturally flow to the bag after the urine tank is full.
6. When the urine bag is almost full, open the drainage tap, and discharge the urine into the predetermined container, close the drainage tap and stored again.

Contra-indications:

None

Transport and Storage:

Keep away from high pressure and sunlight and keep dry during transportation. The storage conditions: relative humidity should be less than 80%, shady and cool, dry, clean, draughty, no corrosive gas.

Precautions:

1. This product is for single use, please do not reuse!
2. This product is for single patient use.
3. Before use, please check if the urine drainage bag and inlet tubing is unobstructed.
4. Before use, please ensure the drainage tap is closed.
5. Do not use if product is beyond the date of expiry.

Warnings:

1. Do not reuse, reprocess, or re-sterilize this medical device. Reuse, reprocessing, or re-sterilization may:
    a. adversely affect the known biocompatibility characteristics of the device
    b. compromise the structural integrity of the device
    c. lead to the device not performing as intended
    d. create a risk of contamination and cause the transmission of infectious diseases resulting in patient injury, illness, or death
2. Cannot use the urine drainage bag as a negative pressure drainage bag, the urine drainage bag has an air vent, so the negative pressure does not work!
3. Under normal circumstances, it is recommended to the urine drainage bag once a week (not affected by the season); however, if the urine of the patient is found to have abnormal phenomena such as flocculation, the urine bag should be replaced in time and ensure drainage unobstructed, and take urine for bacterial culture.
4. The used product should be properly disposed according to the local legislations.

Legal manufacturer:

Global SCP Medical Systems Pte. Ltd., Singapore