


Instructions for use


Bedpan Liner and Disposable Support




1. Place bedpan liner into disposable support, ensuring support pillars are aligned.

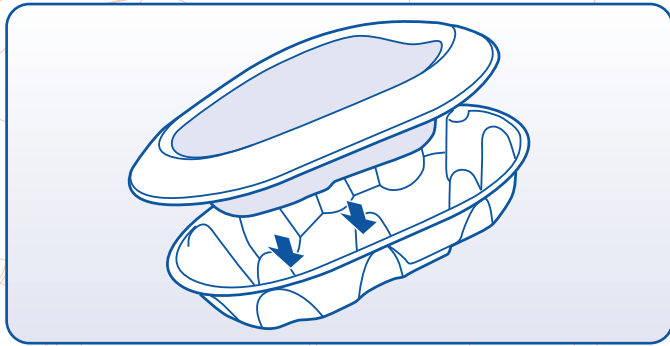


2. Ensure profiling bed is adjusted no higher than a 30° angle to ensure comfortable toileting.

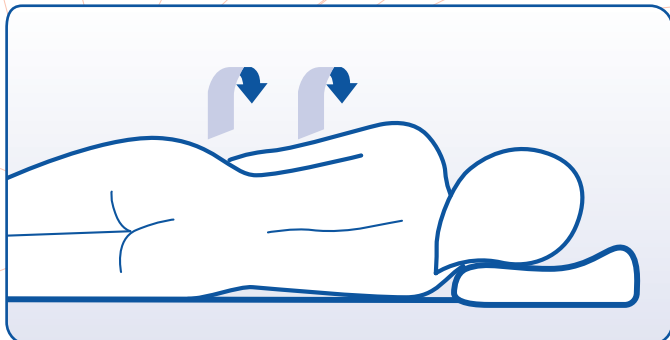

3. Gently roll patient onto their side. A second nurse may be required dependant on the patient condition. (please refer to local policy)

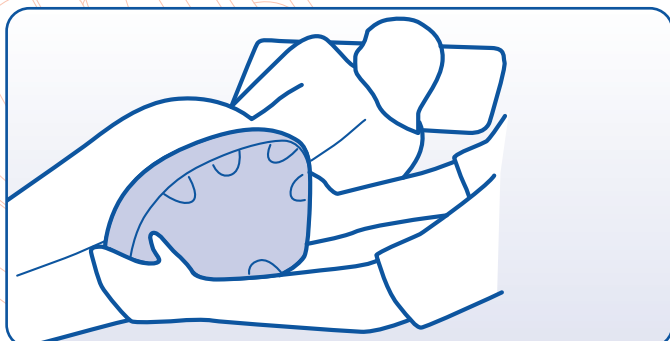

4. Position bedpan liner against patients posterior, ensuring top of the liner is aligned with patient's coccyx to ensure comfort. Gently roll patient back onto the bedpan.

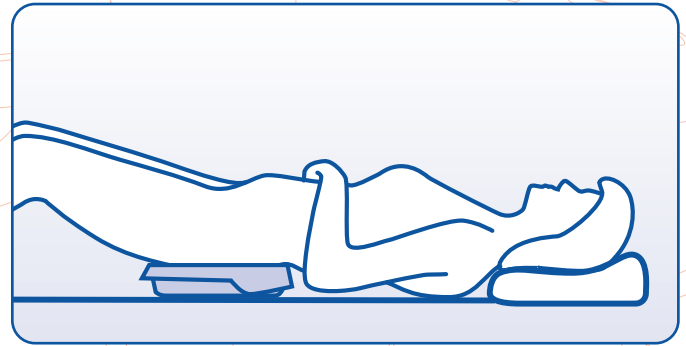

5. Ensure bedpan liner is manoeuvred into comfortable position for patient prior to toileting.



6. After toileting, secure the bedpan liner before gently rolling the patient to one side.





7. Carefully remove the bedpan, using the underside grooves to easily grip the disposable support. At this point, the disposable support can be removed and used as a lid if required.




8. Gently roll patient back into their original lying position and dispose of the bedpan liner and disposable support in the pulp disposal unit.

**How much
does your
patient weigh?**

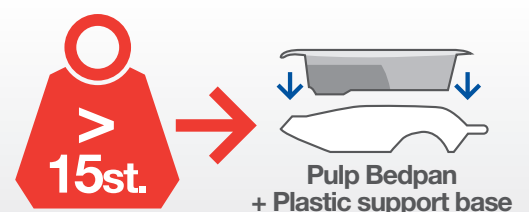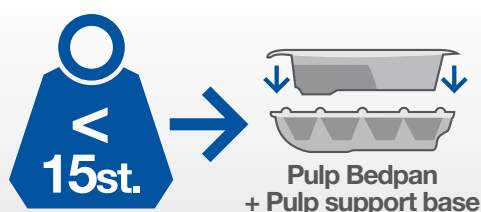

Instructions for use


Bedpan Liner and Disposable Support

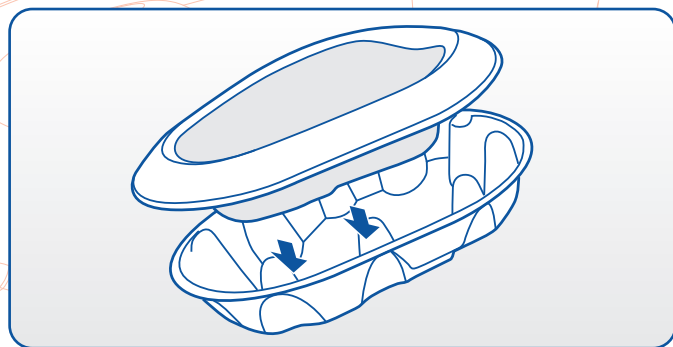


1. Place bedpan liner into disposable support, ensuring support pillars are aligned.




2. Ensure profiling bed is adjusted no higher than a 30° angle to ensure comfortable toileting.

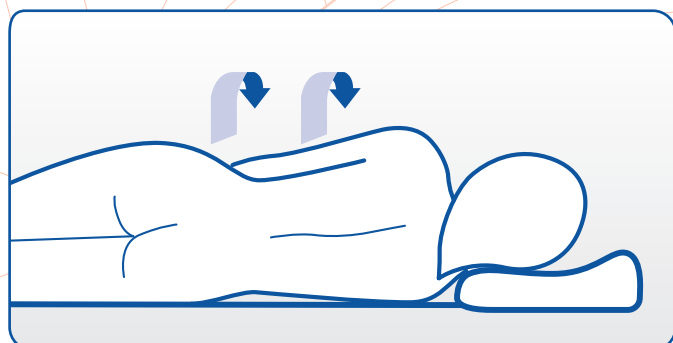

3. Gently roll patient onto their side. A second nurse may be required dependant on the patient condition. (please refer to local policy)

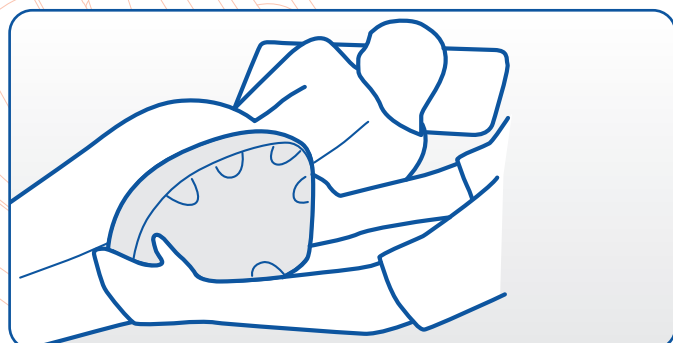

4. Position bedpan liner against patients posterior, ensuring top of the liner is aligned with patient's coccyx to ensure comfort. Gently roll patient back onto the bedpan.

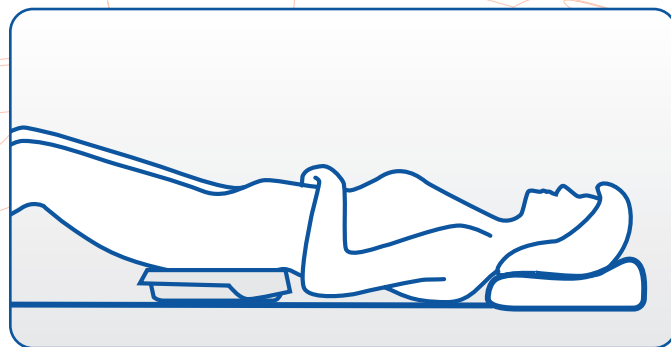

5. Ensure bedpan liner is manoeuvred into comfortable position for patient prior to toileting.



6. After toileting, secure the bedpan liner before gently rolling the patient to one side.




7. Carefully remove the bedpan, using the underside grooves to easily grip the disposable support. At this point, the disposable support can be removed and used as a lid if required.



8. Gently roll patient back into their original lying position and dispose of the bedpan liner and disposable support in the pulp disposal unit.

**How much
does your
patient weigh?**



Pulp Bedpan
+ Pulp support base




Pulp Bedpan
+ Plastic support base

Instructions for use

Bedpan Liner and Disposable Support


Vernacare
cleaner safer healthcare

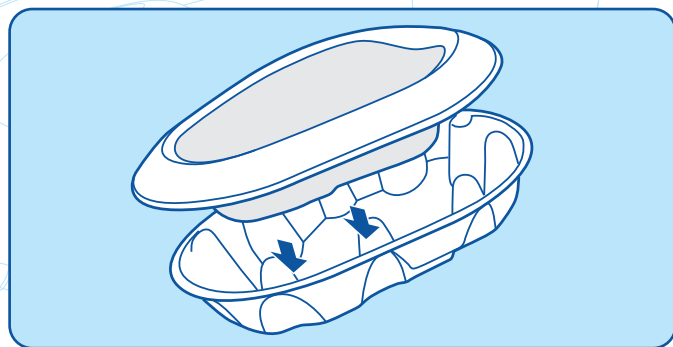

1. Place bedpan liner into disposable support, ensuring support pillars are aligned.




2. Ensure profiling bed is adjusted no higher than a 30° angle to ensure comfortable toileting.

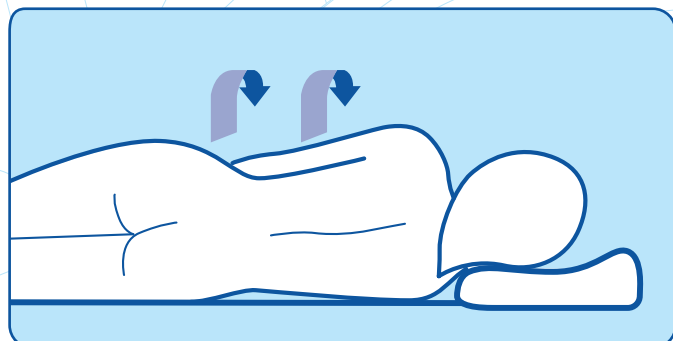

3. Gently roll patient onto their side. A second nurse may be required dependant on the patient condition. (please refer to local policy)



4. Position bedpan liner against patients posterior, ensuring top of the liner is aligned with patient's coccyx to ensure comfort. Gently roll patient back onto the bedpan.

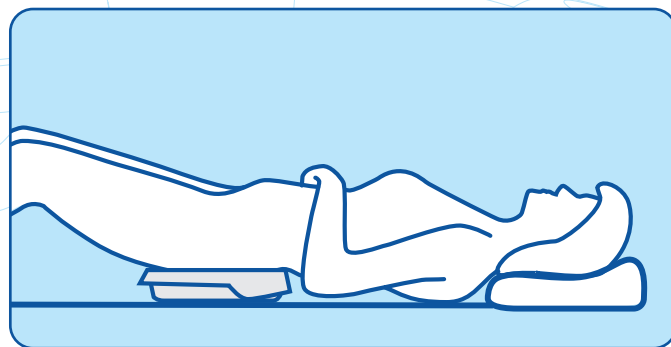

5. Ensure bedpan liner is manoeuvred into comfortable position for patient prior to toileting.



6. After toileting, secure the bedpan liner before gently rolling the patient to one side.




7. Carefully remove the bedpan, using the underside grooves to easily grip the disposable support. At this point, the disposable support can be removed and used as a lid if required.



8. Gently roll patient back into their original lying position and dispose of the bedpan liner and disposable support in the pulp disposal unit.

**How much
does your
patient weigh?**




Pulp Bedpan
+ Pulp support base



Pulp Bedpan
+ Plastic support base

Instructions for use


Bedpan Liner and Disposable Support

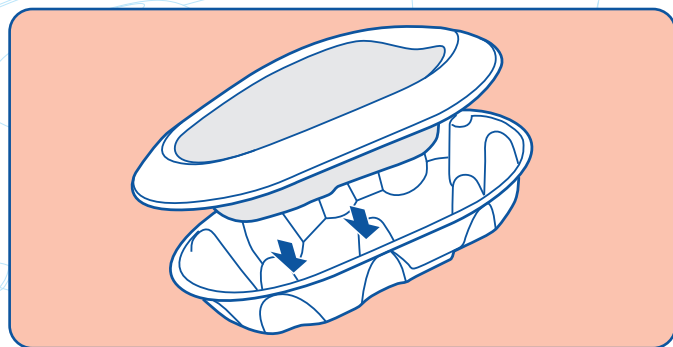


1. Place bedpan liner into disposable support, ensuring support pillars are aligned.




2. Ensure profiling bed is adjusted no higher than a 30° angle to ensure comfortable toileting.

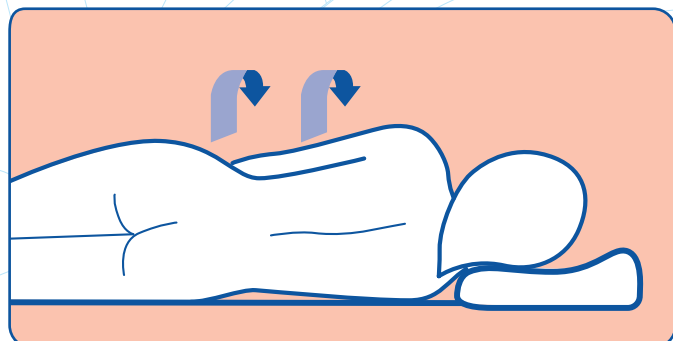

3. Gently roll patient onto their side. A second nurse may be required dependant on the patient condition. (please refer to local policy)

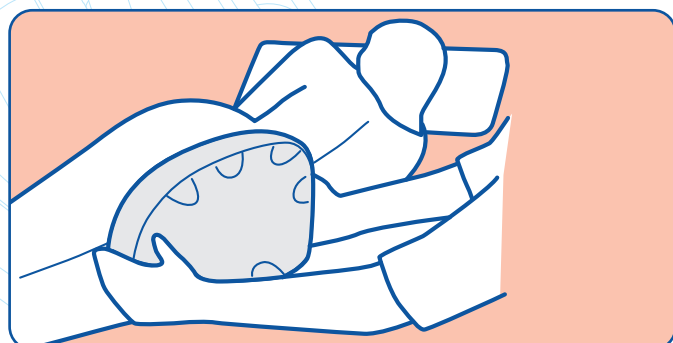

4. Position bedpan liner against patients posterior, ensuring top of the liner is aligned with patient's coccyx to ensure comfort. Gently roll patient back onto the bedpan.

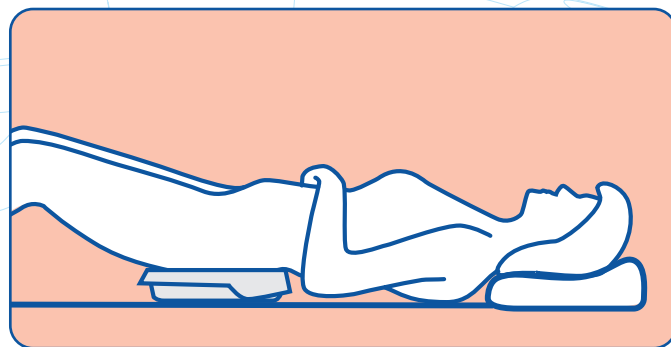

5. Ensure bedpan liner is manoeuvred into comfortable position for patient prior to toileting.



6. After toileting, secure the bedpan liner before gently rolling the patient to one side.




7. Carefully remove the bedpan, using the underside grooves to easily grip the disposable support. At this point, the disposable support can be removed and used as a lid if required.



8. Gently roll patient back into their original lying position and dispose of the bedpan liner and disposable support in the pulp disposal unit.

**How much
does your
patient weigh?**




Pulp Bedpan
+ Pulp support base




Pulp Bedpan
+ Plastic support base

Instructions for use


The Midi and Maxi Slipper pans are designed to make toileting an easier task and the roll technique has proved to be the most effective method for patient comfort. Simply roll the patient onto the pan and roll off again after toileting

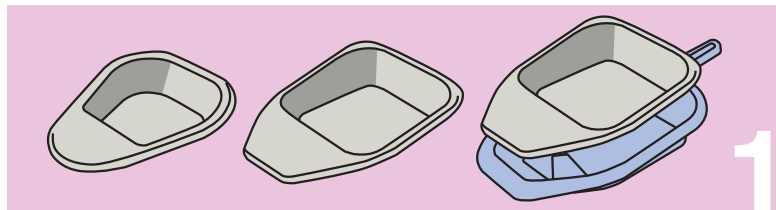


Choose correct size (Midi or Maxi slipper pan available) and place slipper pan liner into support

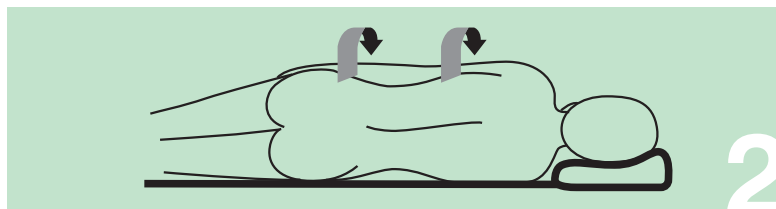


Roll patient onto their side

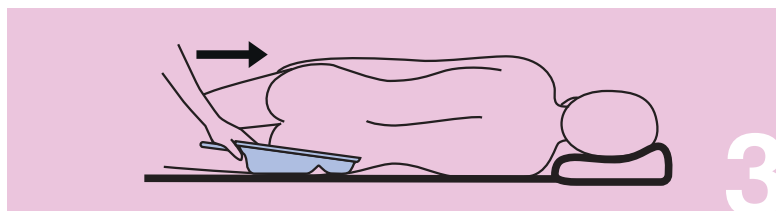

Carefully place slipper pan alongside patient's posterior

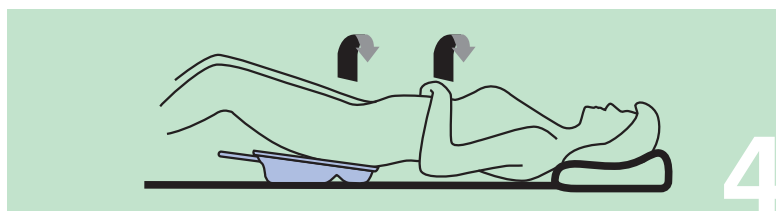


Gently roll the patient onto the slipperpan

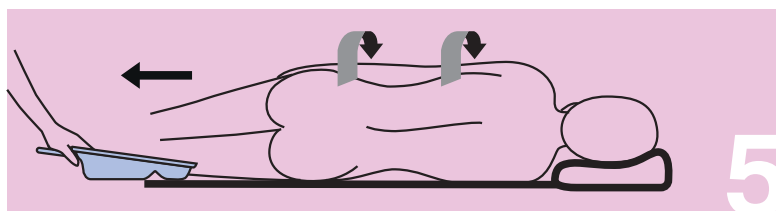

Roll patient onto their side to remove slipperpan and dispose of liner in the macerator


Instructions For Use

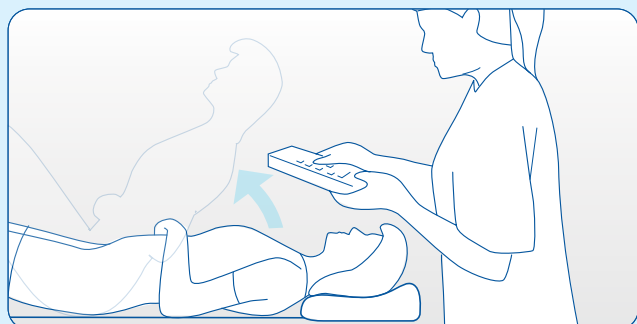


- 1** Adjust profiling bed to ensure patient is comfortable for toileting. Product performance will improve the more upright the patient is positioned.




- 2** Position product, ensuring a comfortable fit up against the patient's body. If the patient is able, they can position the product themselves; therefore increasing confidence, no lifting is required. **Do NOT sit on the product.**

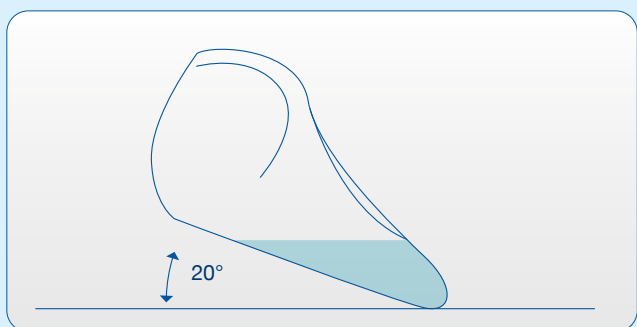


- 3** Product will hold up to 900ml when flat, and up to 350ml at a 20° angle.

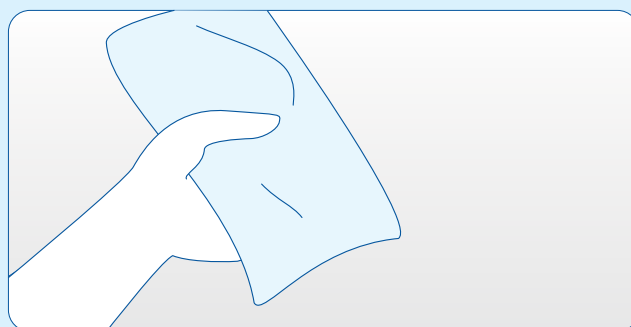

- 4** After toileting, use tissue paper or a soft wipe (ideally maceratable) to wipe away any excess urine.

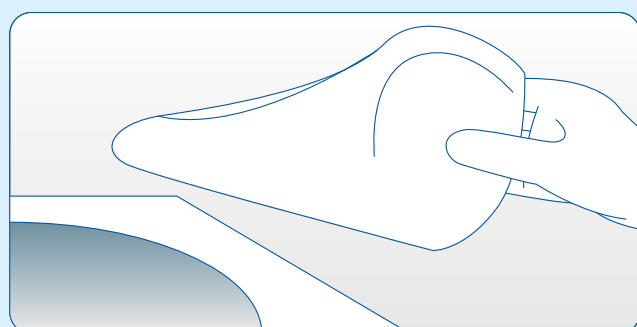

- 5** Carefully remove the product using the handle and dispose in the pulp disposal unit. The VernaFem can also be used to measure urine output.

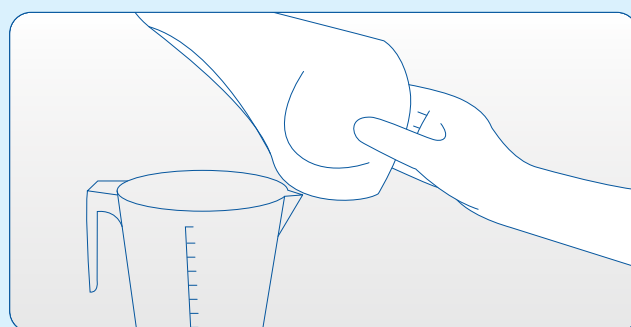

- 6** If required, the handle of the VernaFem can be used to pour the urine into a measuring jug prior to disposal.

Have you also considered?



Senset Dry Wipes
Order Code: 900DY100
Soft, multi-purpose dry wipes
Maceratable
100 wipes



Vernagel Superabsorbent Powder
Order Code: 450MA100
Minimises risk of spillage
Eliminates residual odours
100 x 6g sachets